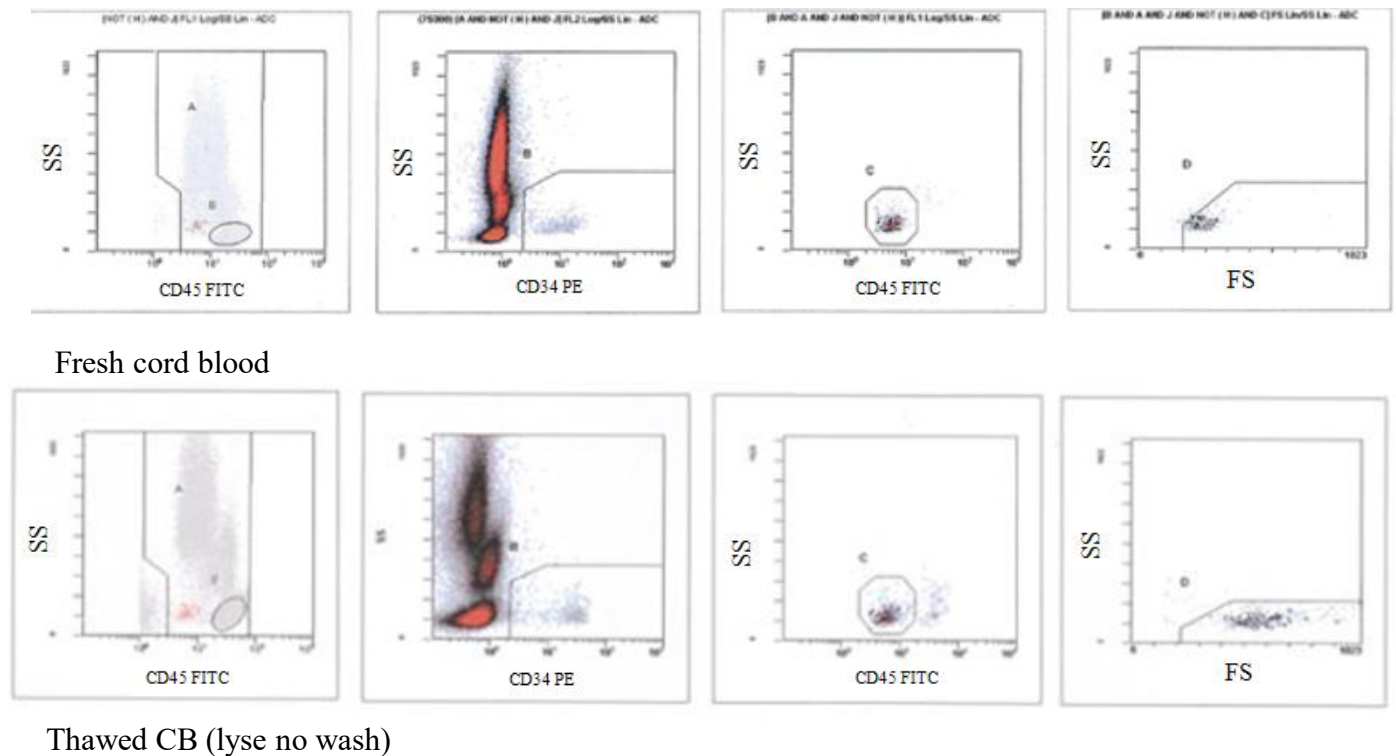


# Single platform cord blood CD34

Vasiliki E. Kalodimou<sup>1\*</sup>

<sup>1</sup>Lab Director at Flow Cytometry-Research & Regenerative Medicine, IASO Maternity & Research Hospital, Athens-Greece



**Figure 1.** Single Platform Cord Blood CD34+ Enumeration: Addition of fluorescent beads of known concentration allows calculation of absolute numbers of CD34+ cells directly from the flow cytometer in fresh and thawed cord blood units.

NOTE: Contaminate an antibody with another antibody will affect the staining profiles, OR bacterial contamination of sheath fluid will result to an increase in the events of flow cytometer.

**Copyright:** ©2017 Kalodimou VE. This is an open-access article distributed under the terms of the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

**Correspondence to:** Vasiliki E. Kalodimou, Lab Director at Flow Cytometry-Research & Regenerative Medicine, IASO Maternity & Research Hospital, Athens-Greece, E-mail: kalodimou@yahoo.gr

**Received:** May 10, 2017; **Accepted:** May 22, 2017; **Published:** May 25, 2017